


COMPONENTS

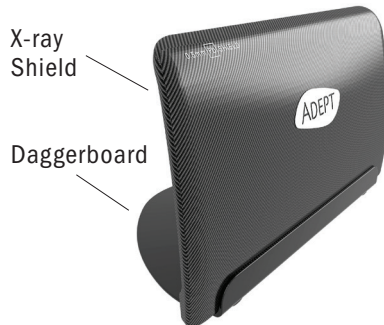


PRODUCT CODE

**AM0500**Daggerboard x 1
X-ray Shield x 1

UNBOXING

①

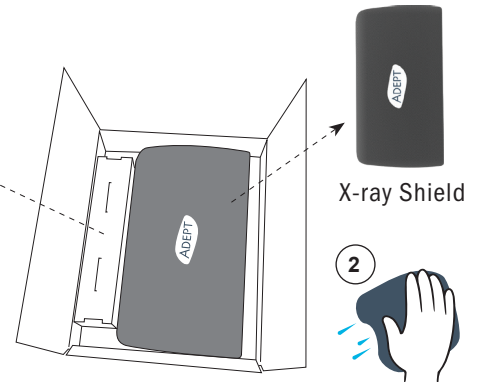


②




SETUP


①

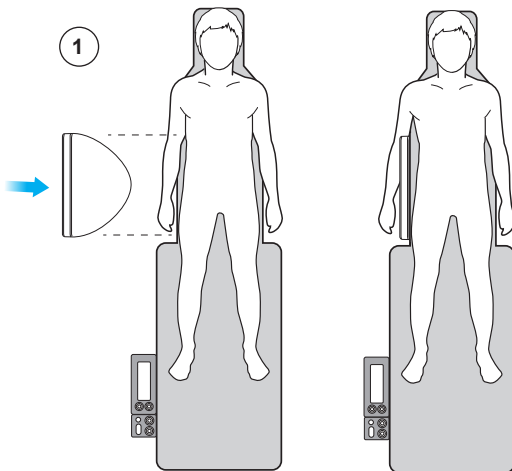


②

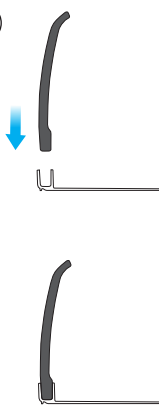

③

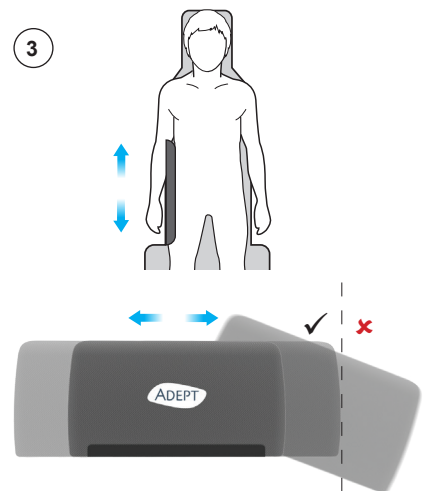

X-RAY

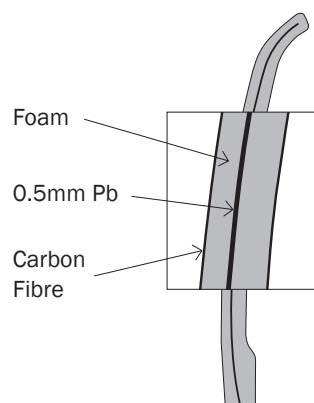For an online training visit:
AdeptMedicalTraining.comFor service and repairs visit
AdeptMedical.com/repairsFor Approved Disinfectants PDF visit:
AdeptMedical.com/ir-system

CLEANING

Disinfect and wipe clean before/after each use.
DO NOT USE any other sterilisation methods.

MANUFACTURER

Adept Medical Ltd
2-6 McDonald St, Morningside
Auckland, New Zealand
www.adeptmedical.co.nz

EC REPRESENTATIVE

Emergo Europe
Prinsessegracht 20
2514 AP The Hague
The Netherlands